
Toenail Correction Device

Composition: The device consists of elastic hooks, fixing pads, a cushioning pad, and an elastic ring. Supplied non-sterile.

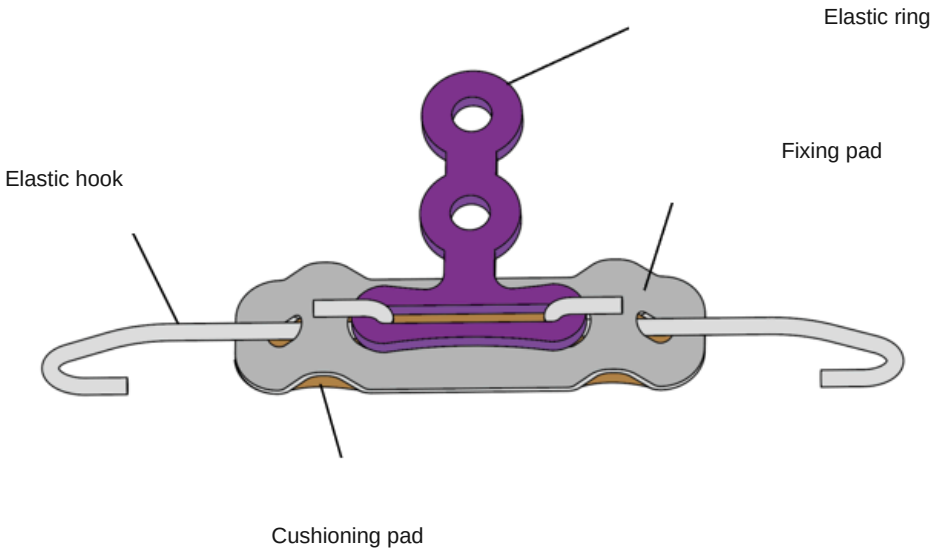

Toenail Correction Device

Classification: **Class II Medical Device**

Classification Code: **09-04**


Intended Use: **Non-invasive correction and adjunctive treatment of ingrown toenails and inflammation of the periungual soft tissue caused by ingrown toenails.**

Supplied non-sterile

Zhejiang Province Class II Innovative Medical Device

Product Name	Toenail Correction Device
Models / Specifications	12 models, differentiated by elastic-hook size, number of correction devices, and fixing-pad thickness: YN-JZ-A2S, YN-JZ-A2M, YN-JZ-A2L, YN-JZ-B2S, YN-JZ-B2M, YN-JZ-B2L, YN-JZ-A4S, YN-JZ-A4M, YN-JZ-A4L, YN-JZ-B4S, YN-JZ-B4M, YN-JZ-B4L.
Product Description	Composed of elastic hooks, fixing pads, a cushioning pad, and an elastic ring.
Intended Use	For non-invasive correction and adjunctive treatment of ingrown toenails and inflammation of the periungual soft tissue caused by ingrown toenails.
Classification Notice	Based on the classification application materials submitted by the company and relevant National Medical Products Administration documents, this product is managed as a Class II medical device. Classification code: 09-04.

Public Notice of Review Results for Zhejiang Class II Innovative Medical Device Special Review Applications (No. 3, 2026) — original document

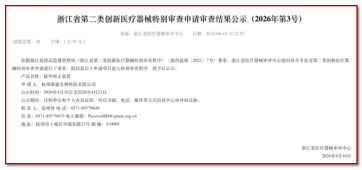
浙江省第二类创新医疗器械特别审查申请审查结果公示（2026年第3号）

Clinical Trial

A multicenter clinical trial is being conducted, with planned enrollment of 80 patients.



浙江大学医学院附属邵逸夫医院伦理审查批件

Ethics Committee Approval Letter of Sir Run Run Shaw Hospital, Zhejiang University School of Medicine

Ethics Committee Approval Letter — original document




INSTRUCTIONS FOR USE

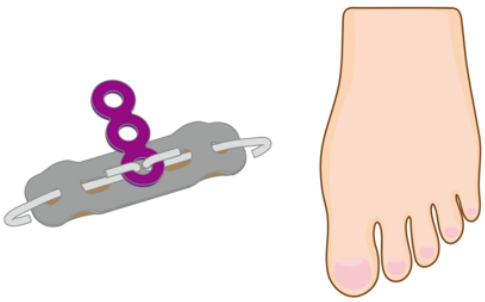


Step 1

Select the appropriate model according to the patient's toenail width. Clean the nail surface with an alcohol swab.

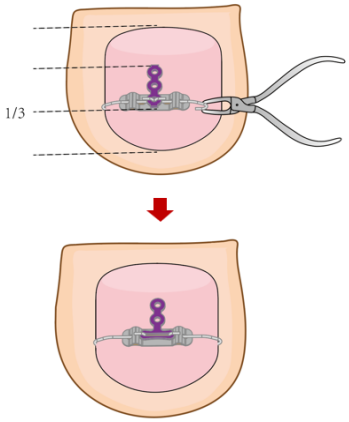


Step 2

Secure one elastic hook to one side of the toenail, near the distal third of the nail, hooking it under the nail plate. Grip the other elastic hook with forceps and fit it over the opposite side of the toenail.



Step 3


Fine-adjust the fixing pads so their midpoint stays over the highest point of the nail's convex surface.

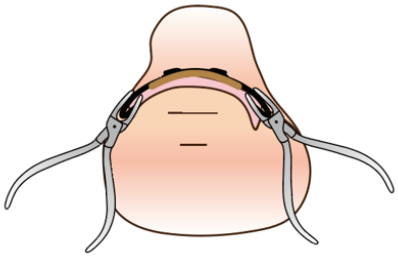

Step 4

Use forceps to adjust the overall position of the correction device, ensuring close contact with the nail surface.

Step 5

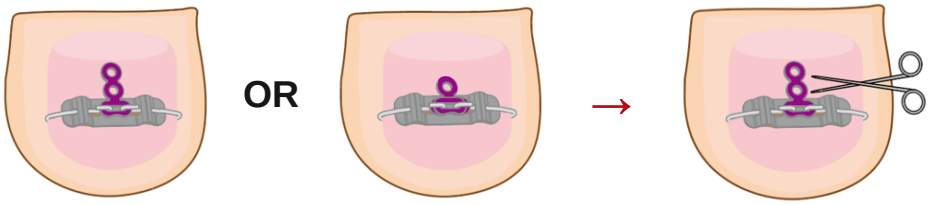

One loop | Two loops

Adjust the number of elastic-ring loops according to the patient's comfort. Appropriate tension produces a slight pulling sensation when the toe is pressed down after application. Trim any excess elastic ring after the procedure.

Hangzhou ORIGOBIO Biotechnology Co., Ltd.

COMPANY ADDRESS
3rd Floor, Building 3, No. 265 Chengrui Street, Xiasha Subdistrict, Qiantang District, Hangzhou, Zhejiang Province, China

TELEPHONE
0571-88313603 / 85150061

EMAIL
disai@decell.cn